

检 测 报 告

Test Report

样品名称 Sample Name: 压力传感器

委托单位 Client: 深圳万讯自控股份有限公司森纳士分公司

生产单位 Manufacturer: /

检验类别 Test Type: 委托检验

无锡科睿检测服务有限公司
Wuxi RELLAB Testing Services Co., Ltd.



在线扫码获取验证

检测报告 Test Report

委托单位/Client:	深圳万讯自控股份有限公司森纳士分公司
委托单位地址/Address:	江阴市花东路 66 号
收样日期/Receipt Date:	2020/11/05
检测项目/Test Item:	IP66
检测周期/Test Periods:	2020/11/05~2021/11/09
检测依据/Test Method:	GB/T4208-2017
检测结论/Conclusion:	详见后续页
备注/Remark:	本报告仅对所测样品有效，未经本实验室同意，部分复制本报告无效。
以下样品信息由委托单位提供并确认 (The following sample information were submitted by client) :	
样品名称/Sample Name:	压力传感器
样品数量/Sample Quantity:	5 件
型号/规格/Type/Model:	DG2
其他样品信息/Other Sample Information:	/
生产单位/Manufacturer:	/

编制:	刘杰	日期:	2020/11/10
Edited by	<u>刘杰</u>	Date	
审核:	秦施炜	日期:	2020/11/10
Reviewed by	<u>秦施炜</u>	Date	
批准:	张大伟	日期:	2020/11/10
Approved by	<u>张大伟</u>	Date	



签发日期: 2020年11月10日
Signature Date Y M D

检测报告 Test Report

一 检测项目/Test Item: IP66

1 检测环境/Test Ambient:

温度: (22~28)°C 相对湿度: (45~70) %RH

2 检测地点/Test Area:

江苏省无锡市滨湖区高浪东路 999 号 A1 栋 检测室

3 检测设备/ Test Instruments:

表 1 检测设备

序号	设备名称	设备管理号	计量有效期
1	砂尘试验箱	WXR002	2020/04/15~2021/04/14
2	防水试验机	WXR023	2020/08/19~2021/08/18

4 检测结果/Test Result:

判定依据: GB/T4208-2017

表 2 测试结果

第一位表征数字为 6	试验结果
防止接近危险部件 用直径 1.0mm 试验金属线, 对产品施加 1N 的力进行试验, 试验金属线不得进入外壳, 并与带电部件保持足够的间隙。	1.1N, 试具未进入壳内
防尘试验 试验应在防尘箱中进行。密闭试验箱的粉末循环泵可用能使滑石粉悬浮的其它方法代替。滑石粉应用金属方孔筛滤过。金属丝直径为 50 μm, 筛孔尺寸为 75 μm。滑石粉的用量按每立方米试验箱体积为 2kg, 使用次数应不超过 20 次。 试验时, 被试外壳按正常工作位置放入试验箱内, 与真空泵连接, 压力不能超过 2kpa (20 毫巴), 持续 2h。 试验后, 样品不能有粉尘进入。	试验后, 样品内无尘进入

第二位表征数字为 5	试验结果
<p>用标准喷嘴，从实际可能的各个方向向试品喷水，条件如下：</p> <p>喷嘴内径：12.5 mm，</p> <p>喷水率：100L/min</p> <p>试验时间：外壳表面每平方米喷水 1min，至少 3 min</p> <p>喷嘴距离：至外壳表面距离 2.5~3m</p>	<p>试验后，样品内无水浸入</p>

5 样品照片/Sample photo:



图 1 样品接收态外观代表性照片



IP6X

IPX6

图 2 样品试验过程中代表性照片

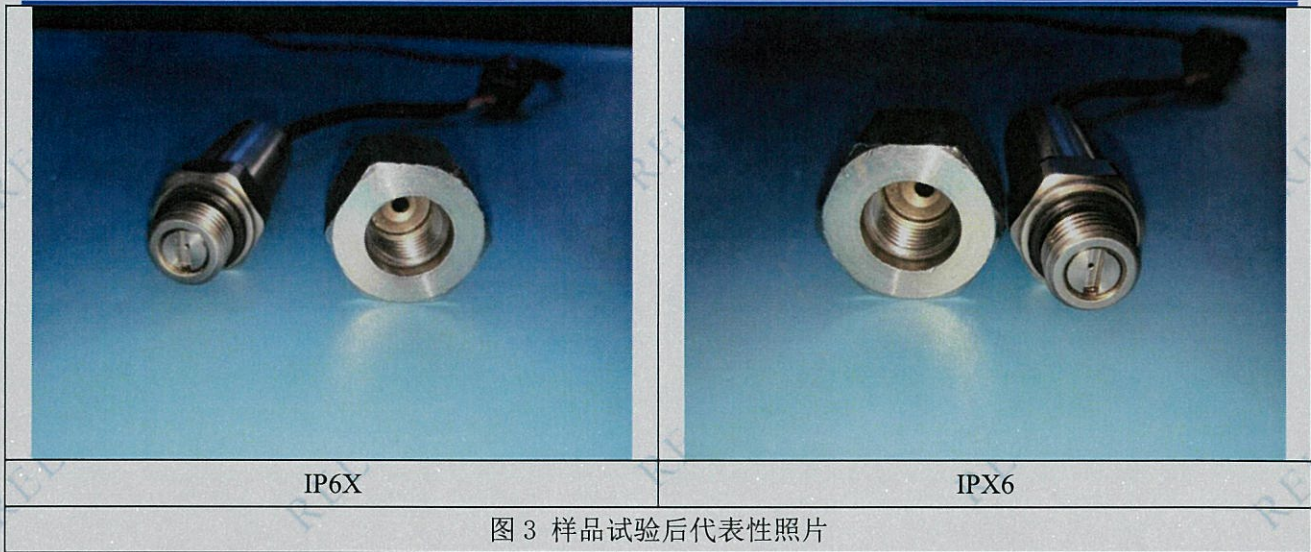


图 3 样品试验后代表性照片

---报告结束/The End---

注意事项

Attention

- 1 报告未加盖本公司“报告专用章”无效。
The report is invalid without "Special Report Seal" of the company.
- 2 未经本公司许可，不得部分复制本报告。
This report is not allowed to be partially copied without our company's permission.
- 3 复制报告未重新加盖本公司“报告专用章”无效。
The copied report is invalid without "Special Report Seal" of the company.
- 4 报告无编制人、审核人、批准人签字无效。
The report is invalid without all signatures of the persons who prepared, supervised and approved.
- 5 报告涂改、自行增删无效。
The report is invalid with self-modification, addition and deletion.
- 6 只对来样的测试结果负责。
The company is only responsible for the results of the sample sent by client.
- 7 本公司对检测报告中的所有信息负责，委托方提供的信息（含数据）除外，当委托方提供的信息（含数据）可能影响本公司检测结果有效性时，特此作免责声明。
The company is responsible for all the information in the test report, except the information (including data) provided by the entrusting party. When the information (including data) provided by the entrusting party may affect the validity of the test results of the company, the company hereby makes a disclaimer.
- 8 如对检测报告有异议，应于收到报告之日起 15 个工作日内向本公司提出申诉，逾期不予受理。
If there is any objection to the report, client shall lodge a complaint with the company on the 15 working days from the date of receipt of the report. No late application will be accepted.
- 9 报告无 CMA 标识时，可作为科研、教学、内部质量控制等活动使用，不具社会证明作用。
The report can be used as scientific research, teaching, internal quality control and other activities without CMA marking, and has no social proof function.
- 10 送检样品务必在收到本检测报告两个月内领取，逾期由本公司自行处理，法律法规、技术文件特殊规定除外。
Samples submitted for inspection must be received within two months after receiving this test report, and the overdue samples shall be handled by our company, except for the special provisions of laws and regulations and technical documents.